


# MODEL 1000 SP

## User Manual

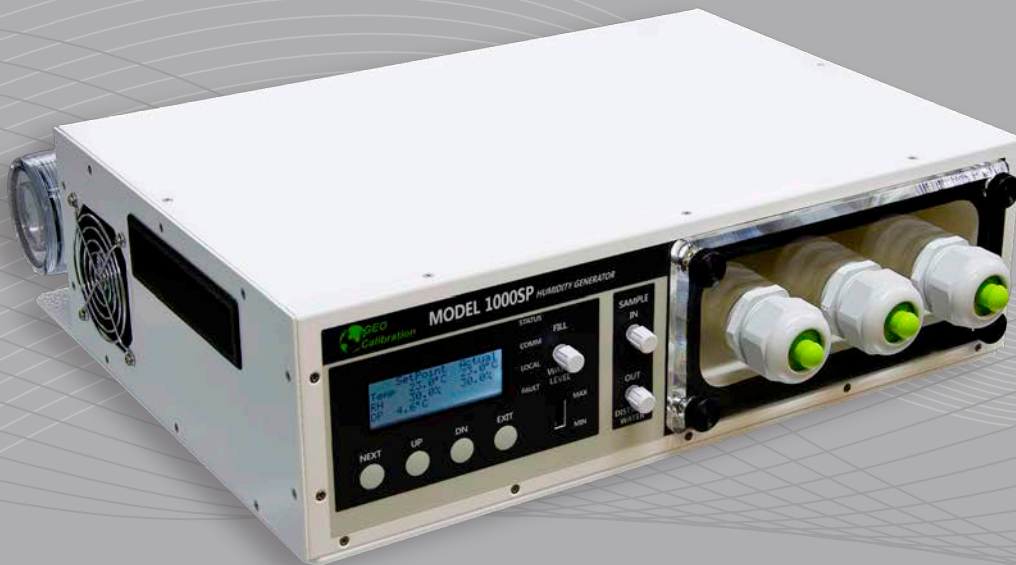

English

Deutsch

Francais

# TABLE OF CONTENTS

<b>INTRODUCTION</b> .....	<b>4</b>
PRODUCT WARRANTY .....	5
UNPACKING INSTRUCTIONS .....	6
CALIBRATOR APPLICATIONS .....	6
STANDARD PACKING CHECK LIST .....	7
STANDARD PACKING CHECK LIST .....	8
VISUAL ITEM CHECK LIST .....	9
ACCESSORY BAG CONTENTS .....	10
ACCESSORY BOX CONTENTS .....	11
AVAILABLE ACCESSORIES.....	12
UNIT DIAGRAM AND PARTS LISTING .....	15
<b>QUICK START GUIDE</b> .....	<b>16</b>
VIDEO VERSION .....	16
FILLING THE RESERVOIR .....	18
POWERING THE UNIT.....	20
UNIT OPERATION (PID CONTROLLER).....	21
ENTERING TEMP & RH SET-POINTS .....	23
BUTTON OPERATION .....	23
STATUS LIGHTS .....	24
UNIT SCREEN NAVIGATION .....	25
CHANGING THE DOOR / OPENING THE CHAMBER .....	27
GENERAL SPECIFICATIONS .....	28
CONSUMABLES.....	29
MECHANICAL .....	29
<b>CALIBRATION</b> .....	<b>30</b>
UUTs (UNITS UNDER TEST) .....	30
CONTROL / REFERENCE PROBE CONFIGURATION .....	31
TWO-POINT CALIBRATION - CLEAR OFFSETS, SLOPE AND INTERCEPT .....	32
TWO-POINT CALIBRATION - TEMPERATURE .....	33
TWO-POINT CALIBRATION - HUMIDITY .....	34
TWO-POINT CALIBRATION - VERIFICATION .....	34
SYSTEM UNCERTAINTY .....	35
AUTO-CALIBRATION   PC SOFTWARE .....	35
<b>REFERENCE STANDARD RECALIBRATION</b> .....	<b>36</b>
Control Probe / Reference Sensor .....	36
<b>ENTERING MODEL 1000 SP OFFSETS</b> .....	<b>38</b>
Unit Offset Calibration via PuTTY .....	38
Accessing the Device Manager .....	38
Reading the COM Port.....	39
Installing PuTTY .....	39
PuTTY Setup .....	39

Connecting Through PuTTY .....	40
Reading Temperature and Humidity Offsets .....	40
Changing Humidity and Temperature Offsets .....	41
<b>SAFETY WARNING .....</b>	<b>42</b>
GENERAL SAFETY INFORMATION .....	42
DISPOSAL SAFETY INFORMATION .....	43
<b>TECHNICAL SUPPORT .....</b>	<b>43</b>
<b>REPAIRS .....</b>	<b>44</b>
UNIT REPAIR PROCEDURES .....	44
<b>MAINTENANCE .....</b>	<b>45</b>
SERVICE SCHEDULE .....	45
ERROR CODES AND DESCRIPTIONS .....	45
DESICCANT CHANGE VISUAL GUIDE .....	46
REPLACING THE CANISTER .....	47
REFILLING DESICCANT CANISTER .....	49
DRAINING THE RESERVOIR .....	50
CONDENSATION IN THE CHAMBER .....	51
CHANGING THE CONTROL PROBE .....	52



GEO Calibration Inc  
2190 Smithtown Avenue, Ronkonkoma, NY 11779, USA  
Tel.: +001 (631) 471 - 6157 • Fax: +001 (631) 471 - 6158  
support@geocalibration.com • www.geocalibration.com

# INTRODUCTION



## MESSAGE FROM GEO CALIBRATION

Thank you for purchasing the GEO Calibration Model 1000 SP humidity and temperature generator/calibrator. We look forward to providing you the highest quality technical support as you become familiar with your new humidity and temperature calibrator.

To better familiarize yourself with the Model 1000 SP, please [visit our Youtube Channel by searching GEO Calibration for user friendly videos.](#)

To start using your GEO Model 1000 SP immediately, you may proceed to our [Quick Start Guide \(page 16\).](#)

For a deeper review of the Model 1000 SP, See our [Calibration Technical Recommendations \(page 28\).](#)

Regards,  
GEO Calibration Service Team

### WARNING

As you read through this product manual, please familiarize yourself with our recommended best practices. By following the proper procedures, you will ensure your unit consistently performs to its highest potential.



Once you have removed the Model 1000 SP from its external packaging, please visually inspect the unit for damage. If damage is found, please immediately contact your supplier.

# LIMITED WARRANTY AND LIMITATION OF LIABILITY

Each GEO Calibration product is warranted to be free from defects in material and workmanship under normal use and service. The warranty period is one year and begins on the date of shipment. Parts, product repairs, and services are warranted for 90 days. This warranty extends only to the original buyer or end-user customer of a GEO Calibration authorized reseller, and does not apply to fuses, disposable batteries, desiccants, distilled water, or to any product which, in GEO Calibration's opinion, has been misused, altered, neglected, contaminated, or damaged by accident or abnormal conditions of operation or handling.

GEO Calibration authorized resellers shall extend this warranty on new and unused products to end-use customers only but have no authority to extend a greater or different warranty on behalf of GEO Calibration. **Warranty support requires activation and registration at:**

<https://www.geocalibration.com/register>

and is purchased through a GEO Calibration authorized sales outlet or Buyer has purchased unit directly from GEO Calibration. GEO Calibration reserves the right to invoice Buyer for importation costs of repair/replacement parts when product purchased in one country is submitted for repair in another country. GEO Calibration's warranty obligation is limited, at GEO Calibration's option, to refund of the purchase price, free of charge repair, or replacement of a defective product which is returned to a GEO Calibration authorized service center within the warranty period.

To obtain warranty service, contact your nearest GEO Calibration authorized service center to obtain return authorization information, then send the product to that service center, with a description of the difficulty, postage and insurance prepaid (FOB Destination). GEO Calibration assumes no risk for damage in transit. Following warranty repair, the product will be returned to Buyer, transportation prepaid (FOB Destination). If GEO Calibration determines that failure was caused by neglect, misuse, contamination, alteration, accident, or abnormal condition of operation or handling, including over voltage failures caused by use outside the product's specified rating, or normal wear and tear of mechanical components, GEO Calibration will provide an estimate of repair costs and obtain authorization before commencing the work. Following repair, the product will be returned to the Buyer, shipped Ex Works FOB Suffolk County NY.

THIS WARRANTY IS BUYER'S SOLE AND EXCLUSIVE REMEDY AND IS IN LIEU OF ALL OTHER WARRANTIES, EXPRESS OR IMPLIED, INCLUDING BUT NOT LIMITED TO ANY IMPLIED WARRANTY OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE. GEO CALIBRATION SHALL NOT BE LIABLE FOR ANY SPECIAL, INDIRECT, INCIDENTAL, OR CONSEQUENTIAL DAMAGES OR LOSSES, INCLUDING LOSS OF DATA, ARISING FROM ANY CAUSE OR THEORY.

Since some countries or states do not allow limitation of the term of an implied warranty, or exclusion or limitation of incidental or consequential damages, the limitations and exclusions of this warranty may not apply to every buyer. If any provision of this Warranty is held invalid or unenforceable by a court or other decision-maker of competent jurisdiction, such holding will not affect the validity or enforceability of any other provision.

GEO Calibration Inc.  
2190 Smithtown Avenue  
Ronkonkoma, NY, 11779  
U.S.A.

## UNPACKING INSTRUCTIONS

Once you have removed the Model 1000 SP from its external packaging, please visually inspect the unit for damage. If damage is found, please immediately contact your supplier.

## CALIBRATOR APPLICATIONS

The GEO Model 1000 SP Humidity Calibrator generates and maintains a controlled humidity and temperature environment for the purpose of testing or calibrating humidity and temperature sensors, also known as hygrometers. The humidity calibration range is 5% up to 95%, while the temperature range is from 5°C to 55°C.

[See the full technical specifications \(page 28\).](#)

The system's accuracy is achieved via a NIST traceable internal control and reference probe.

The Model 1000 SP can calibrate many hygrometer types:

- Probes
- Data-loggers
- Chart Recorders
- Additional Assorted Hygrometers

Please review the dimensions of the calibration chamber to ensure compatibility with the size requirements of any hygrometers you intend to calibrate. You may require an Expansion Chamber. Your GEO representative should have reviewed this with you at time of purchase, if not, please contact our support team and they will size an Expansion Chamber accordingly.

The Model 1000 SP allows for multiple types and sizes of hygrometers, for a complete list please contact us at [support@geocalibration.com](mailto:support@geocalibration.com).



Humidity Control Company

GEO Calibration Inc

2190 Smithtown Avenue, Ronkonkoma, NY 11779, USA  
Tel.: +001 (631) 471 - 6157 • Fax: +001 (631) 471 - 6158  
[support@geocalibration.com](mailto:support@geocalibration.com) • [www.geocalibration.com](http://www.geocalibration.com)

## STANDARD PACKING CHECK LIST

Contents of Shipment			
✓	QTY	Part Number	Description
	1	01-100-00-0000	Model 1000 SP Humidity Generator
	1	01-200-11-0001	Desiccant Canister
	1	01-200-36-0002	Reference Standard / Control Probe
	1	01-200-36-0011	2 Part Desiccant Tool
	1	01-200-01-0013	Desiccant Clamps
	1	01-100-01-0014	1000 SP Accessories Kit
	1	01-200-36-0013	GEO Accessories Box
	1	01-100-07-0001	Model 1000 SP Acrylic Base Plate
	1	N/A	Calibration Documents / Trace Paperwork
	1	1000SP_UM	Model 1000 SP User Manual
	1	N/A	1640 Pelican Case (or equivalent)

Contents of GEO Accessories Kit			
✓	QTY	Part Number	Description
	1	01-200-82-0001	GEO Accessories Bag
	1	01-200-36-0006	Fill Syringe (20ml)
	1	01-200-69-0001	Type A Male to Type A Male USB Cable
	1	01-200-46-0001	Mains Power Cord (220 Vac or 110 Vac)
	1	01-200-30-0001	Banana Jack to Alligator Connectors Red and Black Cable
	2	01-200-85-0001	4 AMP Fuse (1 pack)
	1	01-200-85-0002	1 AMP Fuse (1 pack)

## STANDARD PACKING CHECK LIST

<b>Contents of GEO Accessories Box</b>			
✓	<b>QTY</b>	<b>Part Number</b>	<b>Description</b>
	<b>1</b>	01-001-00-0002	Model 1000SP Door
	<b>4</b>	01-001-66-0001	GEO Knobs (1 pack)
	<b>1</b>	01-200-01-0036	GEO Bunges (7 pack)

<b>Calibration Documents</b>			
✓	<b>QTY</b>	<b>Part Number</b>	<b>Description</b>
	<b>1</b>	NO REORDER	Factory Calibration Report
	<b>1</b>	01-999-99-0001	3rd Party Calibration Certification (IF ORDERED)



## VISUAL ITEM CHECK LIST

Listed below are standard contents included with the purchase of a new Model 1000 SP.



**Humidity Generator**

GEO Calibration  
Model 1000 SP  
P/N: 01-100-00-0000



**Desiccant Canister**

Pre-Filled with molecular sieve  
P/N: 01-200-11-0001



**Control Probe**

HC2-S HygroClip  
control probe (pre-installed)  
P/N: 01-200-36-0002



**Desiccant Tool**

P/N: 01-200-36-0011



**1000 SP Accessories Kit**

Contents:  
See Page 9

P/N: 01-100-01-0014



**1000 SP Accessories Box**


Contents:  
See Page 10

P/N: 01-200-36-0013




**Desiccant Clamps**

P/N: 01-200-01-0013

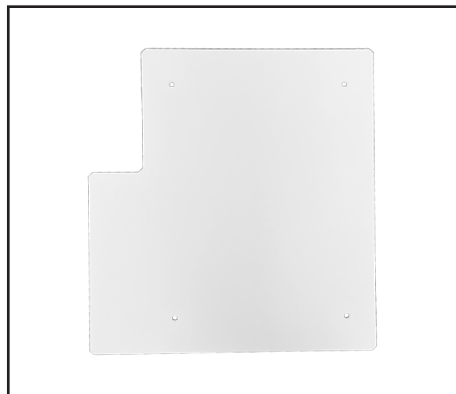


**Model 1000SP Acrylic  
Base Plate**

P/N: 01-100-07-0001

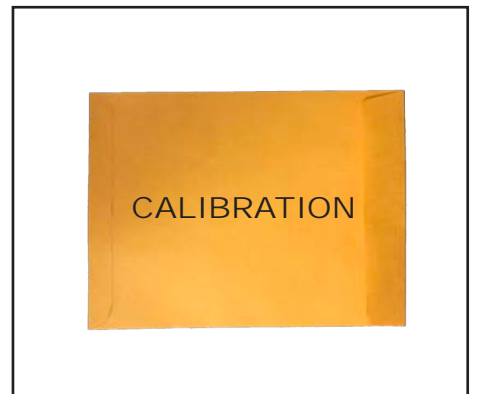


**Calibration Documents**

## ACCESSORY BAG CONTENTS

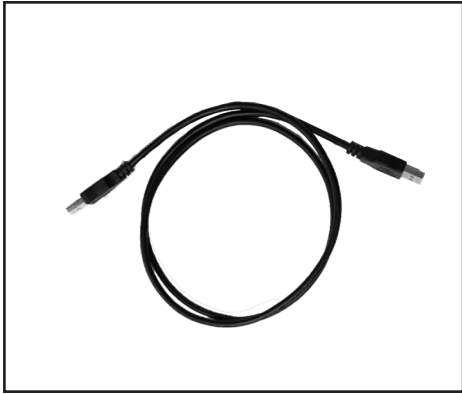

**USB Cable**  
(A to A)

P/N: 01-200-69-0001

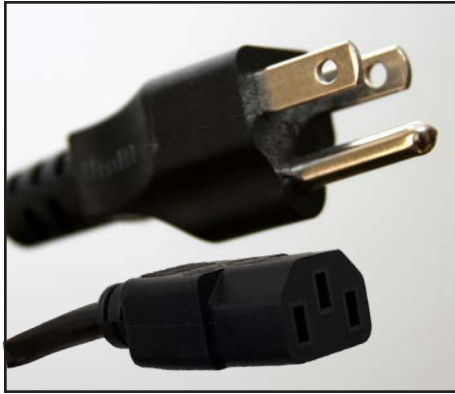

**Mains Power Cord**

P/N: 01-200-46-0001 US  
P/N: 01-200-46-0002 EUR



**Fill Syringe**

P/N: 01-200-36-0006



**Banana Jack to Alligator  
Connectors Red and  
Black Cable**

P/N: 01-200-30-0001



**4 AMP Fuse (2 pack)**

P/N: 01-200-85-0001



**1 AMP Fuse (1 pack)**

P/N: 01-200-85-0002

## ACCESSORY BOX CONTENTS



**Model 1000SP Door**

P/N: 01-001-00-0002



**4 Piece GEO Knob Kit**

P/N: 01-001-66-0001



**7 Piece Bung Kit**

P/N: 01-200-01-0036

## AVAILABLE ACCESSORIES



**Replacement  
Desiccant**

P/N: 01-200-11-0001



**Replacement  
Fill Syringe**


P/N: 01-200-36-0006



**Replacement  
Control Sensor**

HC2-S HygroClip  
control probe

P/N: 01-200-36-0002

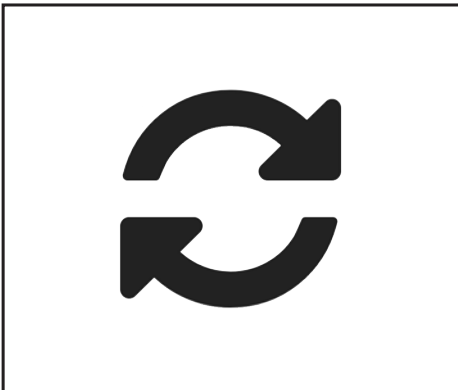

**ISO 17025 System  
Recalibration**

P/N: 01-999-99-0004



**Silicone  
Adapter Variations  
(Regular and Slimline)**

## AVAILABLE ACCESSORIES



Humidity Generator		
QTY	Part Number	Description
1	01-200-11-0001	Desiccant Canister
1	01-200-36-0002	Control Probe
1	01-100-01-0014	1000 SP Accessories Kit
1	01-200-36-0013	GEO Accessories Box
2	01-200-01-0013	Desiccant Clamps
1	01-200-69-0001	USB A to A Cable
1	01-200-46-0001	US Spec Power Cord / Mains Cable
1	01-200-46-0002	EUR Spec Power Cord / Mains Cable
1	01-200-36-0006	Fill Syringe (20ml)
1	01-200-85-0002	1 AMP Fuse (2 pack) (Fast Acting)
1	01-200-85-0001	4 AMP Fuse (2 pack) (Fast Acting)
1	01-200-30-0001	Banana Jack to Alligator Connectors Red and Black Cable
1	01-200-01-0036	7 Piece Bung Kit
1	01-200-36-0011	2 Part Desiccant Tool
1	01-999-99-0001	3rd Party ISO 17025 Calibration Report

## AVAILABLE ACCESSORIES

Grommets / Bungs						
M36 are for Standard Hygrometers PG36 are for Chilled Mirror Adapters						
Part Number	Type		Bung Size		Port Size	
			mm	in	mm	in.
01-004-09-0001	Regular	M36	31.00	1.22"	0.000	0.000"
01-004-09-0002					3.175	0.125"
01-004-09-0003					6.350	0.250"
01-004-09-0004					9.525	0.375"
01-004-09-0005					12.700	0.500"
01-004-09-0006					15.875	0.625"
01-004-09-0007					19.050	0.750"
01-004-09-0008					22.225	0.875"
01-004-09-0009					25.400	1.000"
01-004-09-0020	Slimline	M36	31.00	1.22"	3.175	0.125"
01-004-09-0021					6.350	0.250"
01-004-09-0022					9.525	0.375"
01-004-09-0023					12.700	0.500"
01-004-09-0024					15.875	0.625"
01-004-09-0025					19.050	0.750"
01-004-09-0026					20.950	0.825"
01-004-09-0027					25.400	1.000"
01-004-09-0034	Regular	PG36	44.45	1.75"	00.000	0.000"
01-004-09-0028					12.700	0.500"
01-004-09-0029					15.875	0.625"
01-004-09-0030					19.050	0.750"
01-004-09-0031					25.400	1.000"
01-004-09-0032					31.750	1.250"
01-004-09-0033					34.290	1.350"
01-004-09-0035	Slimline	PG36	44.45	1.75"	9.525	0.375"
01-004-09-0036					15.875	0.625"
01-004-09-0037					25.400	1.00"

# UNIT DIAGRAM AND PARTS LISTING

Below you will find a diagram of the Model 1000 SP's various operational parts.

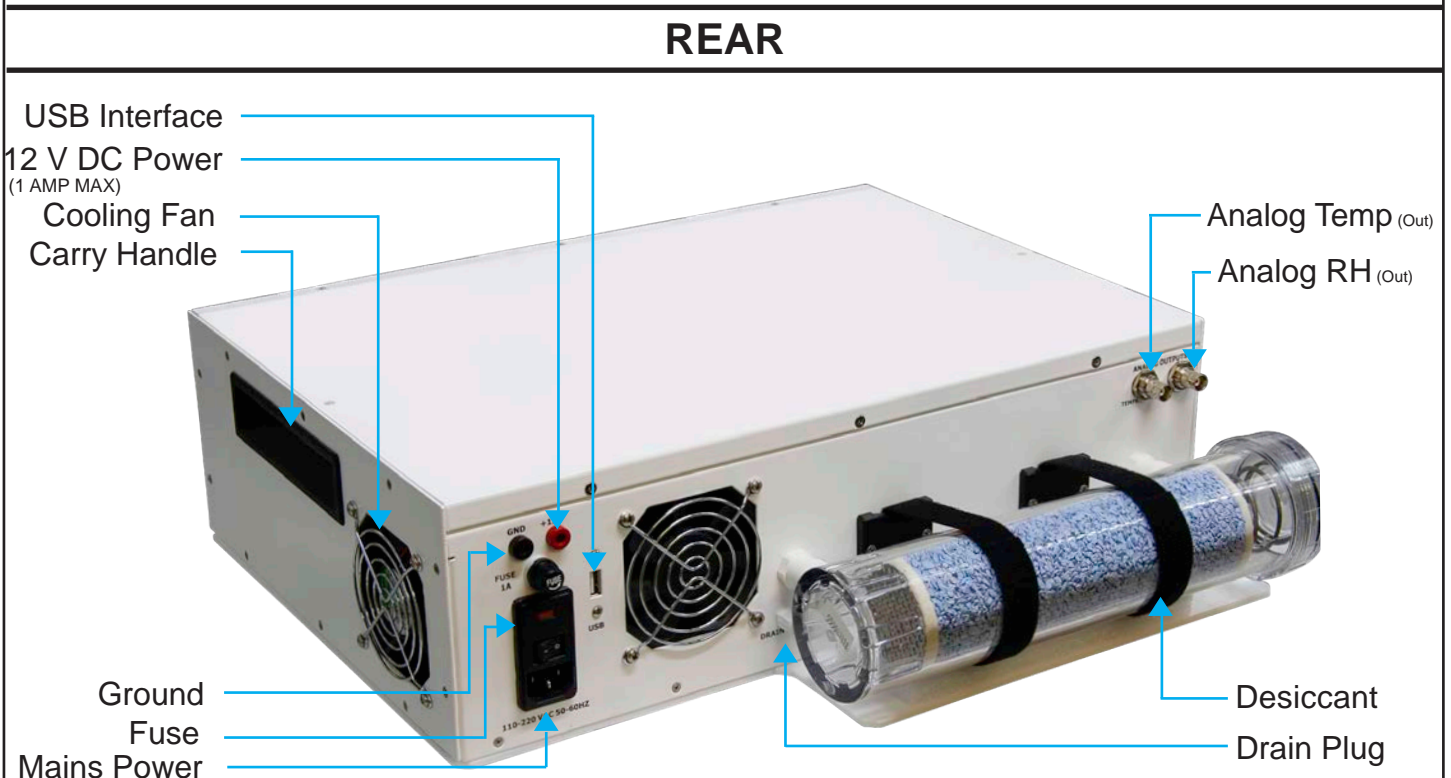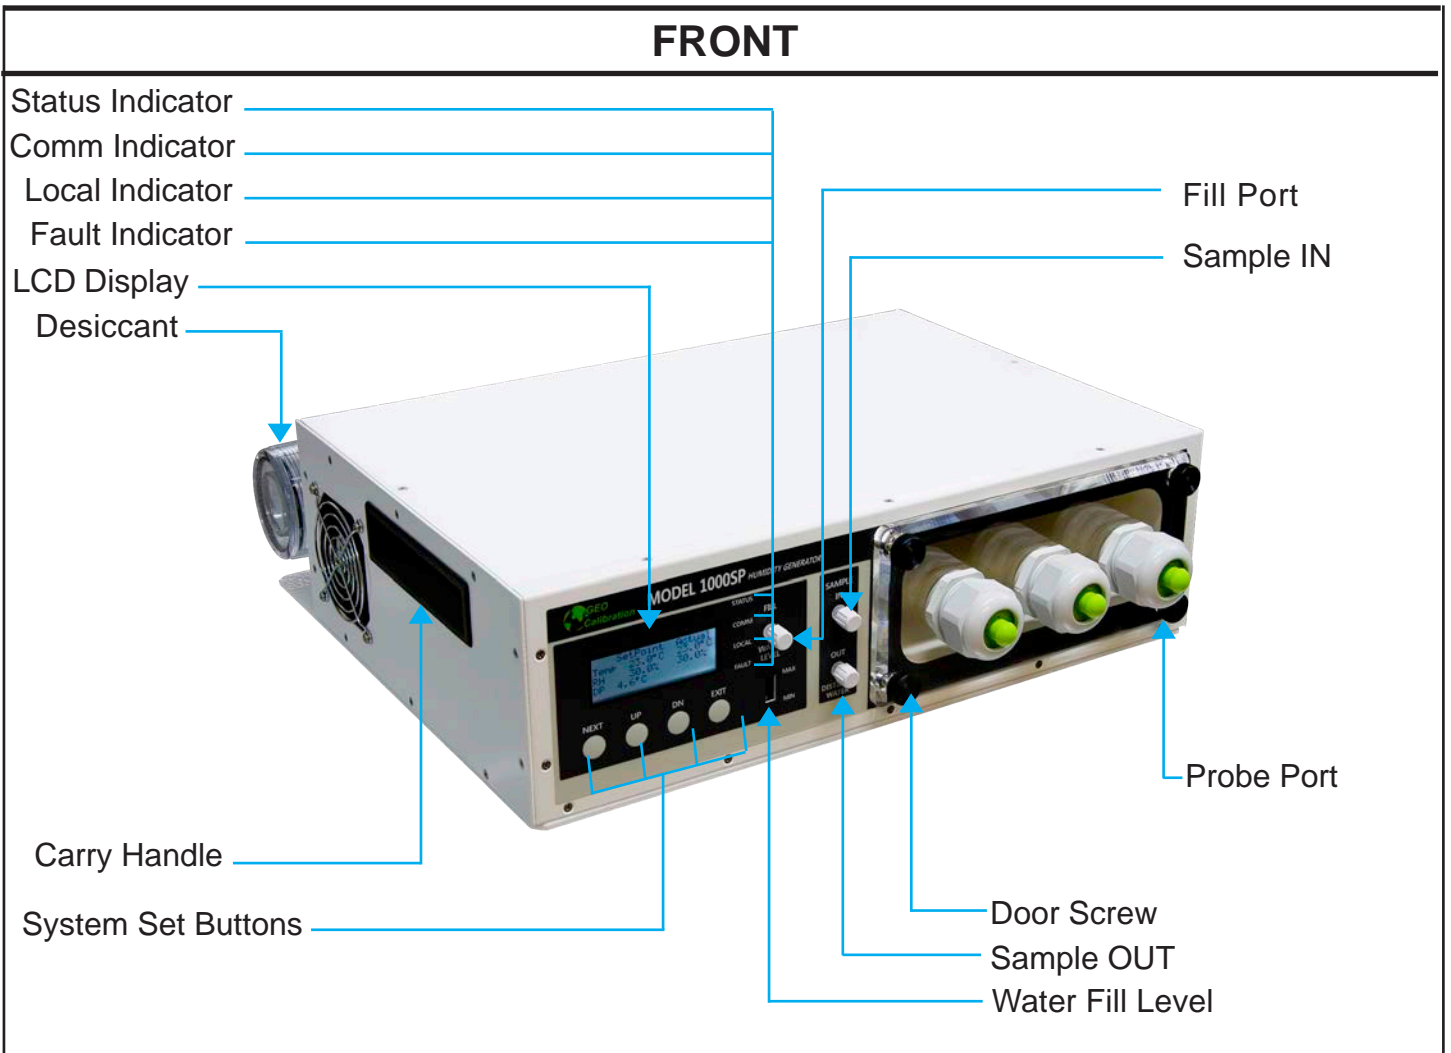

# QUICK START GUIDE

This guide is intended to give you the necessary information to quickly get up and running with your 1000 SP humidity and temperature generator.

It includes the following instructions:

- Filling the Reservoir
- Powering On the Unit
- Operating the Front Panel Controller
- Reading the Status Indicator Lights
- Removing / Changing the Door

## VIDEO VERSION

Visit our website at:

[www.geocalibration.com](http://www.geocalibration.com)

and the YouTube Channel

by searching **GEO Calibration**





# Read Before Turning On The Unit

---

1.

After receiving the unit, open the door to let the chamber dry for 10 minutes. Use soft paper towel to wipe the water in the chamber if needed.

2.

Turn on the unit and set the temperature to 30 °C and humidity to 30 % to let the unit settle, approximately for 20 minutes (first time only).

## PLEASE NOTE:

---

1. Do not use alcohol inside the chamber.
2. The above instruction must be followed to ensure unit is dry from any changes during shipping.

## FILLING THE RESERVOIR

### Supplies Needed

Distilled Water  
Only



Fill Syringe




#### 1. Locate the Fill Port

The port is labeled and located on the middle lower portion of the front panel.




#### 2. Remove the Fill Cap

Rotate Counter-Clockwise to remove.

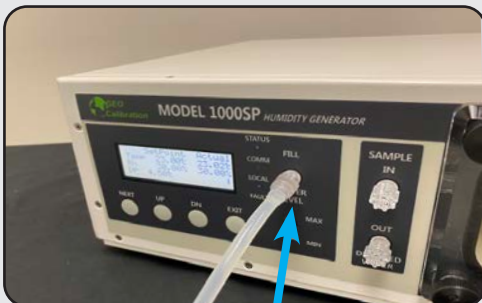


#### 3. Attach Fill Syringe to Fill Port

Press the fill syringe tip into the fill port, then rotate the cap clockwise to secure.

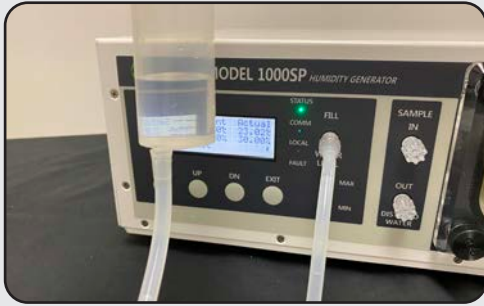


## 4. Elevate and Fill Syringe

- Pour distilled water into the elevated tube body.
- Take care not to insert any air into the reservoir.
- Monitor the water level indicator while filling.

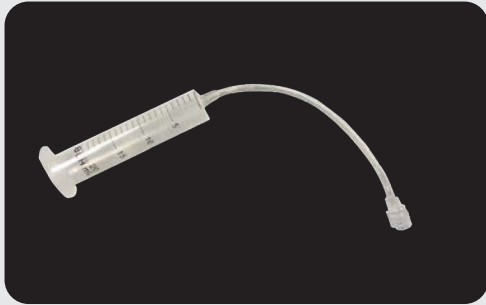

## 5. Loosen and Remove Syringe

Turn the fill syringe tip counter-clockwise to loosen.

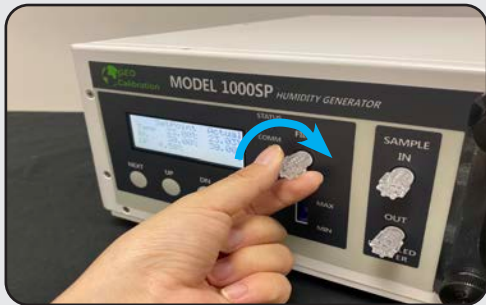

## 6. Re-Install the Fill Cap

Turn the cap clockwise to tighten the cap and seal the fill port.

## POWERING THE UNIT

### Supplies Needed

Mains Power Cord




1. Locate the Power Input



2. Plug Power Supply into Wall

Voltage range is 100 - 260 V AC - 50/60 Hz.  
Total power usage is 240 Watts.

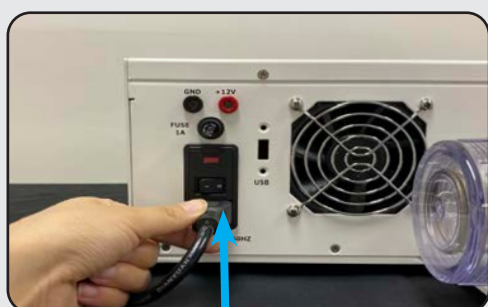


3. Plug Power Supply into Unit



4. Set Power Switch to "ON"

## UNIT OPERATION (PID CONTROLLER)

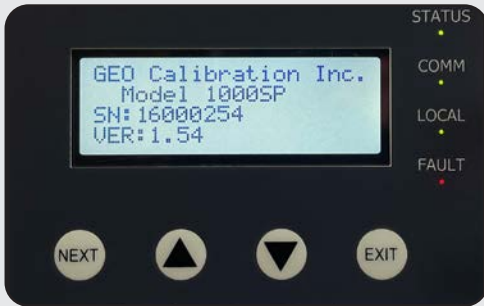


### 1. Boot Screen

**Manufacturer Name**  
**Model Number**  
**Serial Number**  
**Firmware Version Number**




### 2. Observe the Display

<b>Current Temperature</b>	Top Right
<b>Current Relative Humidity</b>	Middle Right
<b>Programmed Temperature</b>	Top Left
<b>Programmed Relative Humidity</b>	Middle Left
<b>Calculated Dew Point</b>	Bottom Left

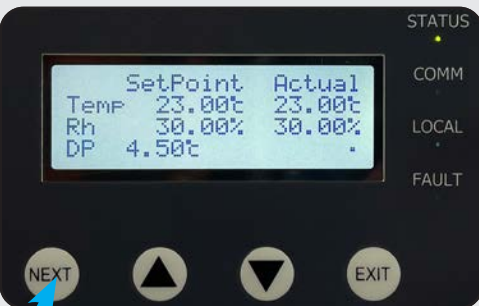


### 3. Changing Humidity & Temperature

Pressing the “Next” button activates the set-point interface. The selected field will repeatedly flash its current programmed value. Repeated presses will toggle between the Humidity and Temperature fields.

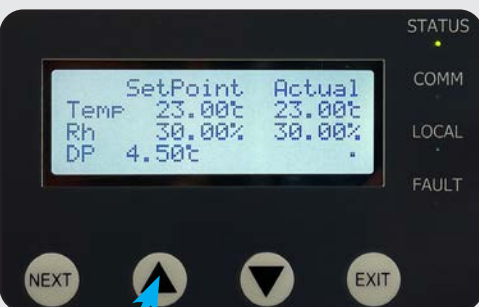

### 4. Raise the Desired Set-point

Pressing the “UP” key will raise the selected set-point. Holding the “UP” key will rapidly raise the selected set-point.

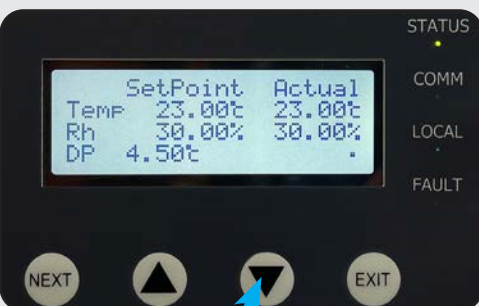

### 5. Lower the Desired Set-point

Pressing the “DN” key will lower the selected set-point. Holding the “DN” key will rapidly lower the selected set-point.



## 6. Commit Your Changes

Pressing the “EXIT” key will commit your changes. It will submit your change after 5 seconds.

## ENTERING TEMP & RH SET-POINTS

From the Main Screen press the 'NEXT' Button. The current set point for temperature will flash indicated in the figure below. If the 'NEXT' Button is pressed again, set point for RH will flash. This means user can change the value of set point by using 'UP' and 'DN' Arrow Button.

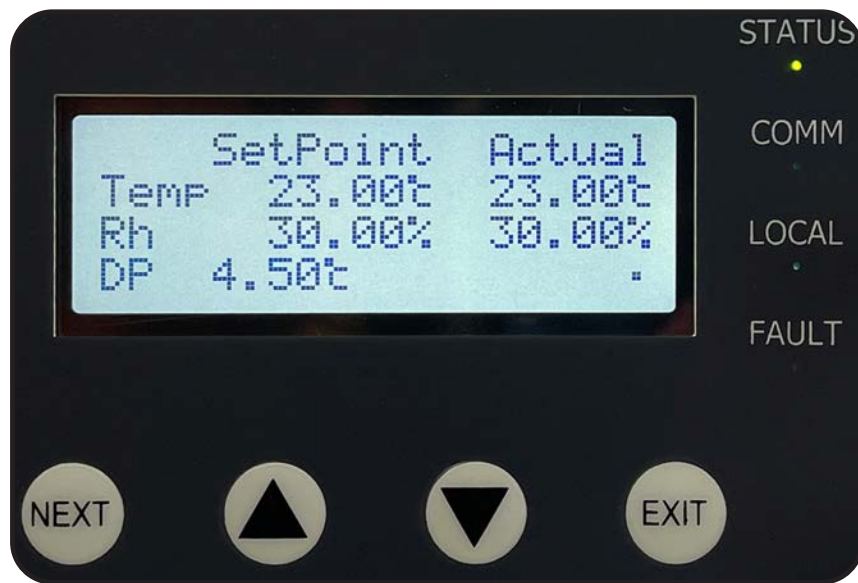


Figure 1 Main menu

## BUTTON OPERATION

The unit has 4 push buttons located below the LCD screen. The push buttons are labeled, 'NEXT', 'UP', 'DOWN' and 'EXIT'.



Figure 2 Push buttons

The 'NEXT' button advances the cursor to either the next user editable value or to the next menu. Depressing the button briefly activates a field into editing mode so that it may be modified. When a field is in edit mode it will flash. To edit the next field on the screen depressing the 'NEXT' button again and the next field will flash indicating it is in edit mode. To exit edit mode either press the 'EXIT' button or wait 30 seconds and the field will automatically exit edit mode.


Holding the 'NEXT' button depressed for more than 10 seconds will advance to the next menu.

The 'UP' button is active when a field is placed in edit mode. Pressing the 'UP' button increases the value of the field while pressing the 'DOWN' button decreases the value. Holding either the 'UP' or 'DOWN' button for more than one second will advance the value of the field at a high rate allowing the user to quickly change a field's value.

Depressing the 'EXIT' button will exit the editing mode. Depressing the 'EXIT' button for 3 seconds will advance to the previous menu.

The 'EXIT' button has one additional use when the Model 1000 SP is first started it may not have sufficient water vapor to allow the setting of higher relative humidity values. In this case the front panel will flash the word 'HEATING'. During this time the unit will NOT control the chamber's temperature or humidity. To bypass this warm up time and go directly to controlling the chamber press the 'EXIT' button on the main screen. The word 'HEATING' will cease flashing and the unit will begin controlling the chamber.

## STATUS LIGHTS

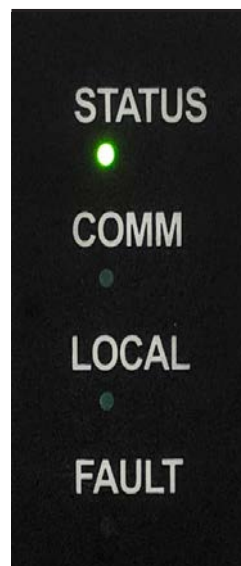

The four status lights located to the right of the LCD screen indicate the following.

The 'STATUS' light indicates the unit is active.

The 'COMM' light indicates the unit is receiving commands from the GEO Model 1000 SP Windows application.

The 'LOCAL' light indicates that the unit's environmental condition is being modified locally from the front panel. That is the current chamber environment has overridden the setting made by the GEO-DFB application.

The 'FAULT' light indicates that the BIT (Built in Test) has detected a condition which will not allow control of the chamber. See appendix Error code for the possible fault conditions.



## UNIT SCREEN NAVIGATION


By pressing the “NEXT” button and holding, user can quickly review the system settings of each screen.



### 1. Main Display

Current Temperature  
Current Relative Humidity  
Programmed Temperature  
Programmed Relative Humidity  
Calculated Dew Point

Top Right  
Middle Right  
Top Left  
Middle Left  
Bottom Left

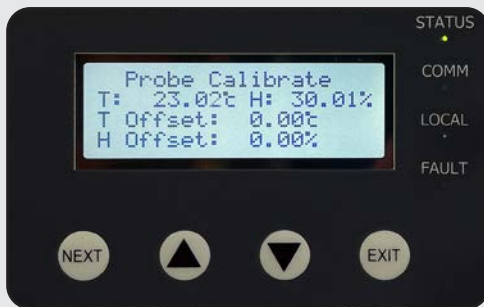

### 2. Probe Calibration

Current Temperature  
Current Relative Humidity  
Temperature Offset  
Humidity Offset

Top Left  
Top Right  
Middle  
Bottom



### 3. Chamber Control

Current Temperature  
Current Relative Humidity  
Override

Top Left  
Top Right  
Bottom




### 4. BIT Heat Exchanger



## 5. BIT Humidity Gen




## 6. Error List

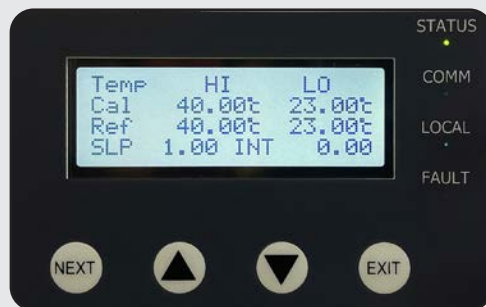

## 7. Two Point Calibration for Temperature

Reading Temperature@40°C	Top Left
Reading Temperature@23°C	Top Right
Reference Temperature@40°C	Middle Left
Reference Temperature@23°C	Middle Right
Temperature Slope	Bottom Left
Temperature Intercept	Bottom Right

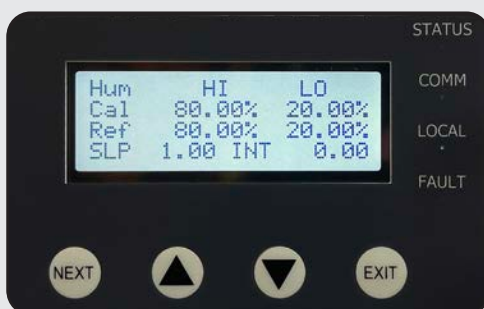

## 8. Two Point Calibration for Humidity

Reading Relative Humidity@80%	Top Left
Reading Relative Humidity@20%	Top Right
Reference Relative Humidity@80%	Middle Left
Reference Relative Humidity@20%	Middle Right
Relative Humidity Slope	Bottom Left
Relative Humidity Intercept	Bottom Right



## 9. Firmware Version

**Manufacturer Name**  
**Model Number**  
**Serial Number**  
**Firmware Version Number**

## CHANGING THE DOOR / OPENING THE CHAMBER



### 1. Unscrew the Corner Screws

Remove screws by turning in a counter-clockwise motion.



### 3. Remove the Door


The best removal method is to pull from the top of the door to break the seal. Once the top is loose, lift and pull to full remove the door.



### 4. Reinstall the Door

# GENERAL SPECIFICATIONS

CALIBRATION TO (17025 TRACEABLE TO NIST)	TRANSFER STANDARD	No Charge	
	CERTIFICATE	17025 Validation (Additional Fees Apply)	
OPERATING AMBIENT CONDI- TIONS	TEMPERATURE	18 °C to 28 °C	
	HUMIDITY	Up to 80 % RH	
STORAGE CONDITIONS	TEMPERATURE	-20 °C to 50 °C	
	HUMIDITY	0 % to 95 % RH (non-condensing)	
ALTITUDE	2000 m		
CALIBRATION SYSTEM ACCURACY	TEMPERATURE	± 0.12 °C Or Better	Typically ± 0.10 °C *Based on Probe Accuracy
	HUMIDITY	± 1.00 % RH Or Better	Typically ± 0.80 % *Based on Probe Accuracy
	CONTROLLER TYPE	PID Controller	
UNIFORMITY	TEMPERATURE	0.10 °C Or Better	Typically ± 0.10 °C
	HUMIDITY	0.30 % RH @ 18 °C to 28 °C Or Better	Typically ± 0.25 %
STABILITY	TEMPERATURE	0.05 °C	
	HUMIDITY	0.15 % RH @ 18 °C to 28 °C	
WARM-UP PERIOD	AMBIENT CONDITIONS	30 Minutes Maximum	
	COLD	30 Minutes	
RESOLUTION	DISPLAY	Temperature	0.01 °C
		Humidity	0.01 % RH
		Dew Point	0.01 °C (Calculated)
	USB	Temperature	0.01 °C
		Humidity	0.01 % RH

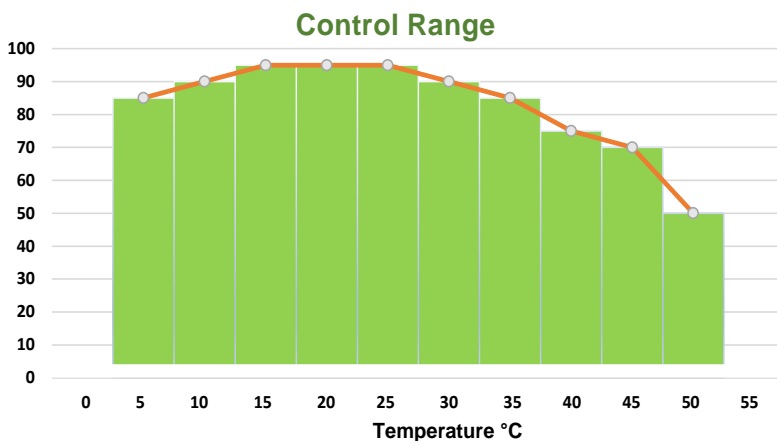

## RAMP / SOAK RATE OF CHANGE

\*Depends on ambient and desiccant conditions

TEMPERATURE	High → Low	1.50 °C / minute *Typical
	Low → High	3.00 °C / minute *Typical
HUMIDITY	High → Low	5.00 % RH / minute *Typical
	Low → High	10.00 % RH / minute *Typical

## CONTROL RANGE

TEMPERATURE	5 °C to 55 °C	
HUMIDITY @ 18°C	5 % to 95 % RH	HUMIDITY @ 35°C 5 % to 85 % RH
HUMIDITY @ 23°C	5 % to 95 % RH	HUMIDITY @ 40°C 5 % to 75 % RH
HUMIDITY @ 30°C	5 % to 90 % RH	HUMIDITY @ 50°C 5 % to 50 % RH

## SPECIFICATION ANNOTATIONS

If the desired humidity set-point is higher than 70%:

- \* Set the temperature to your desired point first, and let the chamber stabilize. Next, set the humidity to the desired set point.
- \*\* To achieve low temperature with high humidity, you must first set the humidity value to 70% or lower, and let the chamber stabilize. Then, set the temperature to the desired set point. This avoids condensation appearing within the chamber.

Note:

If condensation is formed in the chamber:

- A. Open the chamber door and wipe any visible water away with a paper towel.
- B. Set humidity to 30% and temperature to 30 °C then let the unit dry and stabilize.

## CONSUMABLES

WATER	RESERVOIR	200 ml
	SPILL RESISTANT	Yes
	REQUIRED FLUID	Distilled Water Only
	EST. REFILL PERIOD	15 Days to 1 Month (Typical) *Depends on Usage
	FILL INDICATOR	Floating Ball
DESICCANT	TYPE	Molecular Sieve
	REPLACEMENT	When Indicating Desiccant is 3/4 Used
	REPLACEMENT FREQUENCY	Depends Entirely on User Workload
	LOCATION	Back Side Mounted
	FASTENER	Desiccant Mounting Bracket Provided
RECALIBRATION	FREQUENCY	Depends on User Uncertainty Requirements Once Per Year Recommended

## MECHANICAL

GENERATOR DIMENSIONS	Measurement Type	Width	Depth	Height
	Metric	46.00 cm	31.50 cm	15.00 cm
	English	18.11 in	15.16 in	9.26 in
CHAMBER DIMENSIONS	Measurement Type	Width	Depth	Height
	Metric	19.50 cm	13.00 cm	7.45 cm
	English	7.68 in	5.12 in	2.93 in
WORKING DIMENSIONS AND VOLUME	Measurement Type	Width	Depth	Height
	Metric	19.50 cm	13.00 cm	7.45 cm
	English	7.68 in	5.12 in	2.93 in
	Volume	1.5 Liter Effective Working Volume		
WEIGHT	Unit Only	Metric	8.5 kg	
		English	18.74 lb	
POWER SUPPLY FOR EXTERNAL USE	Power Supply	12 Volt DC @ 1A		
STANDARD PORT QUANTITY	Depends on doors	Availability: 3 Ports		
PROBE ANALOG OUTPUTS AVAILABLE	0 - 1 Volt	Temperature	- 40.00 to + 60.00 °C	+ 5.00 to + 60.00 °C
		Humidity	0 to + 100.00 %	+ 5.00 to + 95.00 %

# CALIBRATION

## UUTs (UNITS UNDER TEST)

Port Adapter




## Supplies Needed

UUT  
[ Unit Under Test ]




### 1. Select Port Size Adapter

Measure the diameter of the UUT and select the appropriately sized silicone adapter. Unscrew the Model 1000 SP door and replace the adapter if necessary. Ensure the door is securely fastened to the chamber.

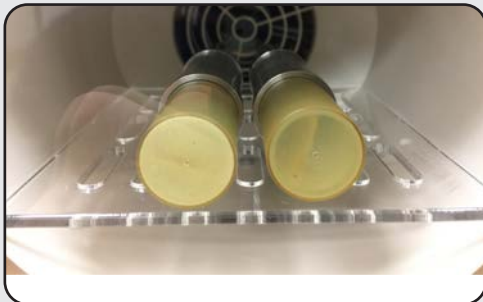

### 2. Insert UUT

Insert your UUT at least 3 inches into the Model 1000 SP chamber.

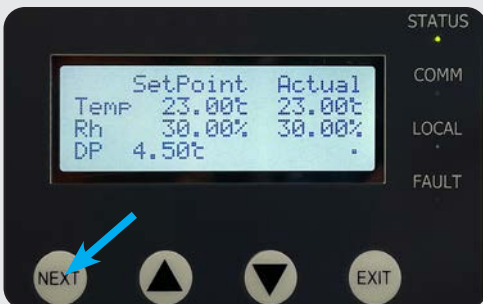

### 3. Program Unit Set-points

Allow the unit to reach the programmed set-points and settle. To best preserve desiccant, it is advised that you begin multi-point calibrations with low humidity set-points.




### 4. Compare Readouts

Follow the manufacturer's recommendation for recalibration and programming offsets.

## CONTROL / REFERENCE PROBE CONFIGURATION

The probe calibration screen allows the user to introduce a calibration offset to the internal probe used to control the GEO Calibration 1000 SP chamber. This allows the user to calibrate the internal probe to an external reference.

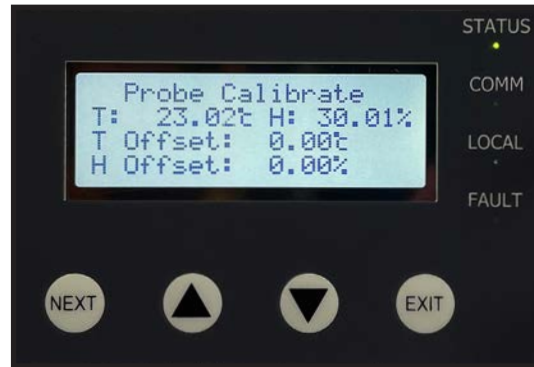

**Figure 5 Control Probe Calibration**


In the image above the current probe offset is 0.1° C and the offset is 0.1% RH. The current chamber temperature and humidity are displayed for reference. Once the offsets are configured the values are permanently stored in the unit and do not need to be reset when the unit is subsequently powered on.

## TWO-POINT CALIBRATION - CLEAR OFFSETS, SLOPE AND INTERCEPT




### 1. Clear Temperature and Humidity - Offsets

1. Clear the temperature offset to a 0.0 °C on Probe Calibration Screen.
2. Clear the humidity offset to a 0.0 % on Probe Calibration Screen.

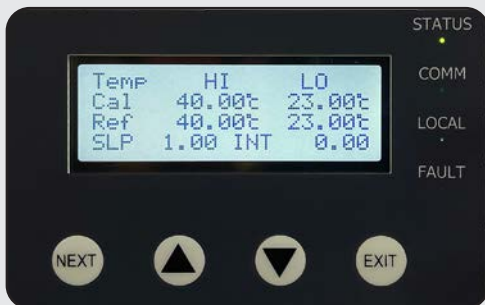

### 2. Clear Temperature – Slope and Intercept

1. Set temperature Ref HI Point to 40 °C and Ref LO Point to 23 °C on Two Point Calibration for Temperature Screen and then press the Exit Button.
2. By doing this the system will clear the Slope and Intercept automatically for temperature.

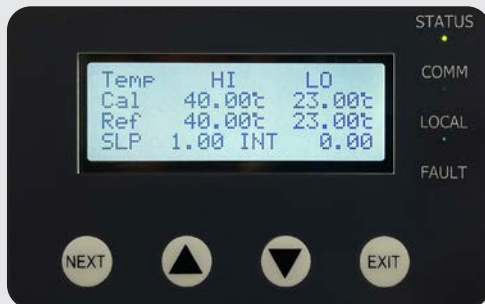

### 3. Clear Temperature – Slope and Intercept (Cont'd)

3. The Slope value will be 1.00 and the Intercept value will be 0.00. This is to clear all previously calibrated settings.



### 4. Clear Humidity – Slope and Intercept

1. Set humidity Ref HI Point to 80% and Ref LO Point to 20% on Two Point Calibration for Humidity Screen and then press the Exit Button.
2. By doing this the system will clear the Slope and Intercept automatically for Humidity.



### 5. Clear Temperature – Slope and Intercept (Cont'd)

3. The Slope value will be 1.00 and the Intercept value will be 0.00. This is to clear all previously calibrated settings.



## TWO-POINT CALIBRATION



### REQUIREMENTS:

- Firmware Version: 1.53 or higher
- High Accuracy Certified Reference Probe inserted into the chamber
- System settings as per page 2 of this document
- Pen and paper to record reference probe readings

### PLEASE NOTE:

GEO recommends the two points calibration are 23 °C and 40 °C for Temperature and 20% to 80% for Humidity. These ranges are the most linear, and probe performance outside of these ranges are less linear.



## TWO-POINT CALIBRATION - TEMPERATURE

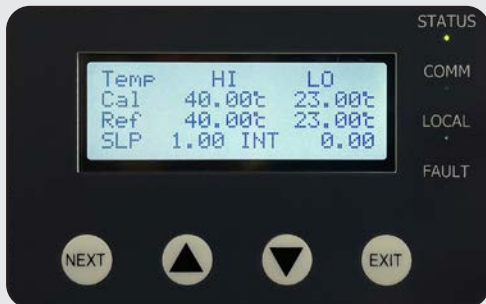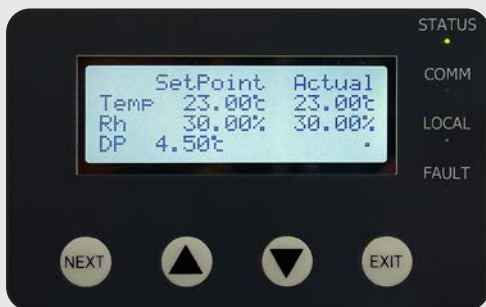

1. Set temperature to 23 °C on Main Display and let the unit settle.
2. Record the readings of your reference probe on paper for later entry.
3. Then set temperature to 40 °C on Main Display and let the unit settle.
4. Record the readings of your reference probe on paper for later entry.
5. Now toggle to Two Point Calibration for Temperature Screen and enter the Ref HI and LO previously recorded values, after entering these values press the EXIT Button.
6. The system will calculate slope and intercept automatically for temperature.



## TWO-POINT CALIBRATION

### TWO-POINT CALIBRATION - HUMIDITY

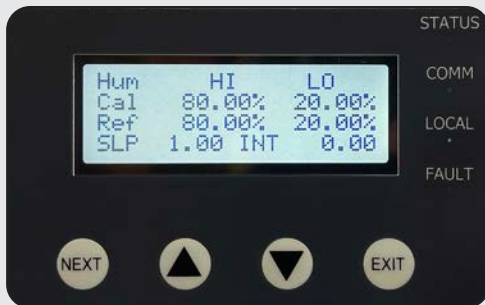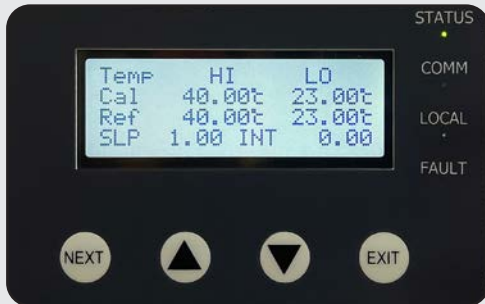

1. Set temperature to 23°C and humidity to 20 % on Main Display and let the unit settle.
2. Record the readings of your reference probe on paper for later entry.
3. Then set humidity to 80 % on Main Display and let the unit settle.
4. Record the readings of your reference probe on paper for later entry.
5. Now toggle to Two Point Calibration for Humidity Screen and enter the Ref LO and HI previously recorded values and press the EXIT Button. The system will calculate slope and intercept automatically for humidity.

### TWO-POINT CALIBRATION - VERIFICATION

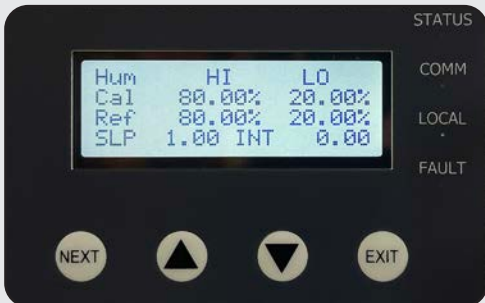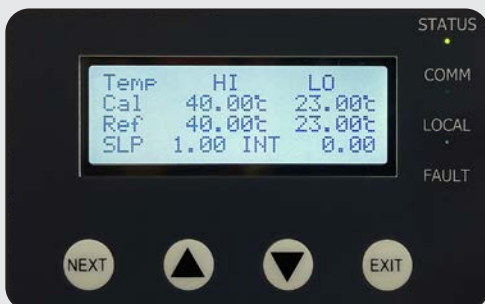

1. Set temperature to any point within the specifications and let it settle down and compare the system conditions with the Reference probe, it should match with in 0.1 °C.
2. Set humidity to any point within the specifications and let it settle down and compare the system conditions with the Reference probe, it should match with in 1.0%.
3. Your Two Point Calibration is complete.

# SYSTEM RECALIBRATION

## SYSTEM UNCERTAINTY

The absolute uncertainty of the system depends on multiple variables:

- **System Warm Up** – All components must be warmed up and stabilized before doing any calibration, as mentioned before, humidity depends on temperature, and the system must stabilize to ambient room conditions before performing calibrations.
- **Uniformity** – Mixing of the humidity and temperature inside the chamber can cause uniformity issues. GEO has a unique chamber design to achieve high uniformity within all GEO chambers.
- **Sensor/Probe Uncertainty** – This is the largest contributor to system uncertainty and that is why system probes are calibrated using instruments and standards traceable to the National Institute of Standards and Technology (NIST).
- **Controller Error** – Our Controllers use PID loops with calculations down to 7 digits. These calculations have fractional errors that can compound if ignored. GEO's proprietary solutions are able to minimize controller error, leaving only a small amount of uncertainty contribution.
- **Hysteresis** – Hysteresis is the system's error based on its usage history. GEO engineers have developed system modeling techniques to significantly reduce hysteresis uncertainties.

## AUTO-CALIBRATION | PC SOFTWARE

Software options are available for licensed users. Please contact GEO Calibration for more information.

Customers not having purchased the license for Auto-Calibration software, please refer to the following pages for unit offset calibration.

# REFERENCE STANDARD RECALIBRATION

## Control Probe / Reference Sensor

### Overview

The Model 1000 SP functions through the use of a dual PID controller. This controller takes the humidity and temperature values from an internal capacitance probe and further performs calculations that are then used to generate the user entered humidity and temperature set points. This sensor is factory calibrated, and upon request, additionally calibrated by an ISO 17025 accredited laboratory using either a chilled mirror or two-pressure primary reference standard.

When calibrating the Model 1000 SP, the chamber must be measured at a variety of temperatures and relative humidity levels. It is recommended applying measurement guardbands to improve system accuracy and reduce any measurement uncertainties. The Model 1000 SP's humidity and temperature offsets must be changed if the control probe's readings are found to be outside of the allowed tolerances when compared to the reference.

### Capacitive Recalibration Intervals

The scope and uncertainty requirements of this calibration will vary per customer. The capacitance probes that we use have an average drift of 1.0% RH per year. You should account for this interval, as well as your laboratory's uncertainty budget when calculating out your desired recalibration interval. The table below illustrates accuracy drift after 6, 12 and 24 months.

Timeframe	6 Months	12 Months	24 Months
Drift (%RH)	0.5% RH	1.0% RH	2.0% RH

Based on this information, you may wish to shorten or lengthen your calibration interval to respectively increase accuracy or decrease costs.

### Chilled Mirror Recalibration Intervals

Chilled mirrors operate by measuring light defraction caused by frost or condensation formation on a mirror. Unless the mirror is damaged, it is not mandatory to recalibrate. It will require periodic cleaning, as per the manufacturer's instructions.

### Internal Capacitive Probe: Self Re-calibration Overview

We advise that you return your capacitive reference probe to GEO Calibration for recalibration. However, for customers that are international or operate where policy restricts the use of international services, self recalibration is an option.

The following supplies are needed to recalibrate the internal capacitive control/reference probe.

HW4 Calibration Software

HygroClip DI Adapter Cable HC2 Pbe/USB, 6Ft

A calibration reference with uncertainties of 0.5% RH or better.

# REFERENCE STANDARD RECALIBRATION



## Self Recalibration Procedure

To read the recalibration procedure of the control / reference probe, please refer to the unit's user manual, and the HW4 software manual found at the following URLs as of publication of this manual:

[https://s.campbellsci.com/documents/ca/manuals/hc2-s3-l\\_man.pdf](https://s.campbellsci.com/documents/ca/manuals/hc2-s3-l_man.pdf)

<https://goo.gl/n7qE1G>

<https://www.instrumart.com/assets/rotronic-hygroclip2-probes-manual.pdf>

Before recalibration of any control probe, ensure that the unit and probe have both completely settled at 23°C for at least ten minutes.

## Maintaining Probe Accuracy

The following text is the recommended maintenance best practices from Rotronic:

The HC2S3 probe requires minimal maintenance, but dust, debris, and salts on the filter cap will degrade sensor performance. Check the white filter on the end of the sensor for debris. If dirt or salt is engrained into the filter, it should be cleaned with distilled water or replaced. Make sure the filter is connected firmly with your fingers — do not over tighten.

Check the radiation shield monthly to make sure it is free from dust and debris. To clean the shield, remove the sensor from the shield. Dismount the shield. Brush all loose dirt off. If more effort is needed, use warm, soapy water and a soft cloth or brush to thoroughly clean the shield. Allow the shield to dry before remounting.

Replace corroded, discoloured or clogged filters. To replace the filter, unscrew the filter from the probe and pull it straight away, being careful not to bend or damage the sensors. Before putting on the replacement filter, check the alignment of the sensors with the probe, and if necessary, carefully correct the alignment before installing the filter.


The Teflon filter is recommended when the sensor is installed in close proximity to the ocean or other bodies of salt water. A coating of salt (mostly NaCl) may build up on the radiation shield, sensor, filter and even the sensors. A build-up of salt on the filter or sensors will delay or destroy the response to atmospheric humidity.

Long term exposure of the relative humidity sensor to certain chemicals and gases may affect the characteristics of the sensor and shorten its life. The resistance of the sensor depends strongly on the temperature and humidity conditions and the length of the pollutant influence.


# ENTERING MODEL 1000 SP OFFSETS

## Supplies Needed

Windows PC with  
USB Port

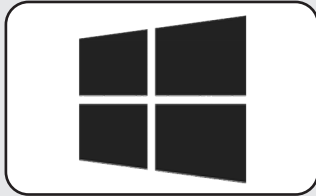

USB Cable

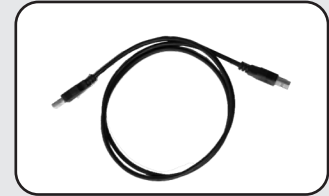

## Unit Offset Calibration via PuTTY

The Model 1000 SP also allows users to make two, single point adjustments for both temperature and humidity. It is recommended that users recalibrate their unit as needed to fit their overall uncertainty requirements.

The reference sensor used for this recalibration should be either a two-pressure or chilled mirror primary measurement standard.


The following software items are required for this recalibration:

- Windows Device Manager
- PuTTY \*

## Accessing the Device Manager

Press and hold the Windows key, tap R, then release both keys.

A Run window will appear. Type **devmgmt.msc** into this window, then hit Enter on your keyboard.

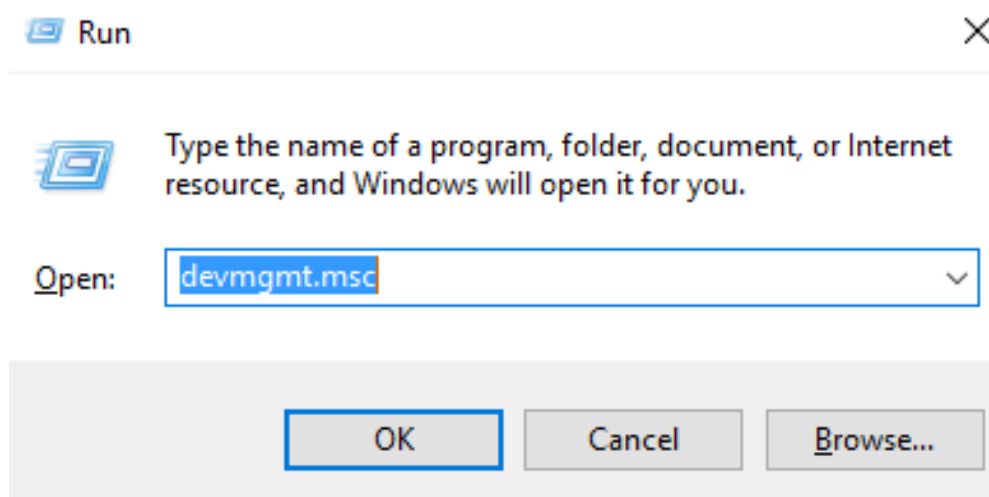

\* PuTTY is a free and open-source terminal emulator. It is distributed under the MIT Software License, and is completely free for unrestricted commercial use. For more details on the PuTTY license, [click here](#).

# ENTERING MODEL 1000 SP OFFSETS

## Reading the COM Port

At this time, plug the unit's power supply into an approved power source.  
Plug the USB mouse and keyboard into the Unit.  
Toggle both the power switches to the "ON" position.

With Device Manager open, expand the Ports (COM & LPT) menu. While watching the expanded Ports sub-menu, plug the free end of the USB cable into the computer. A new entry will appear, called USB Serial Port. To the right of this text, will be parenthesis. Remember the text enclosed within these parenthesis. This is your COM Port, and will be referenced in the following sections.

### Ports (COM & LPT)

Communications Port (COM1)

Communications Port (COM2)

ECP Printer Port (LPT1)

USB Serial Port (COM3)

## Installing PuTTY

Visit [www.ninite.com/putty](http://www.ninite.com/putty) to download the PuTTY installation executable file.


Run the executable and follow the automatic installer instructions to install PuTTY.

Once the installation is complete, run PuTTY by double clicking on the newly created desktop icon.


## PuTTY Setup

Ensure that PuTTY is running on your computer.

From the Category option on the left side of the window, click Terminal menu item to expand the sub-menu.



Under Local echo, select the Force on button



# ENTERING MODEL 1000 SP OFFSETS

## Connecting Through PuTTY

In PuTTY, select **Session** menu under Category on the left

Input your COM Port (reference **Reading the Serial Port** instruction from above) into the **Serial line** field

Under **Connection type**, select **Serial**

Click **Open**

Specify the destination you want to connect to

Serial line: COM3      Speed: 9600

Connection type:  
 Raw    Telnet    Rlogin    SSH    Serial

Load, save or delete a stored session

Saved Sessions: [Empty list]

Default Settings: [Empty list]      [Load]      [Save]      [Delete]

Close window on exit:  
 Always    Never    Only on clean exit

[Open]      [Cancel]

## Reading Temperature and Humidity Offsets

Temperature: type **TOFFSET** and press the enter key. The unit will query and display the temperature offset

```
COM3 - PuTTY
>TOFFSET
Temperature Offset is: 0.1
>
```

Humidity: type **HOFFSET** and press the enter key. The unit will query and display the humidity offset

```
COM3 - PuTTY
>HOFFSET
Humidity Offset is: 0.2
>
```



# ENTERING MODEL 1000 SP OFFSETS


## Changing Humidity and Temperature Offsets

### PLEASE NOTE:

## is a placeholder


In the following instructions, replace # with your desired integers.  
(For example, ## would become 1.2 or -0.2)

Temperature: type **TOFFSET ##** and press the **Enter** key. The unit will query and display the temperature offset. Ensure it has been changed by typing in **TOFFSET** . Press the **Enter** key.

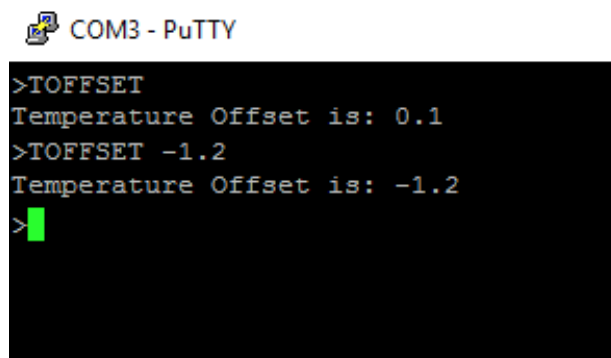

```
COM3 - PuTTY
>TOFFSET
Temperature Offset is: 0.1
>TOFFSET -1.2
Temperature Offset is: -1.2
>
```

Humidity: type **HOFFSET ##** and press the **Enter** key. The unit will set the humidity offset to the new value given by the argument. Ensure it has been changed by typing in **HOFFSET** . Press the **Enter** key.

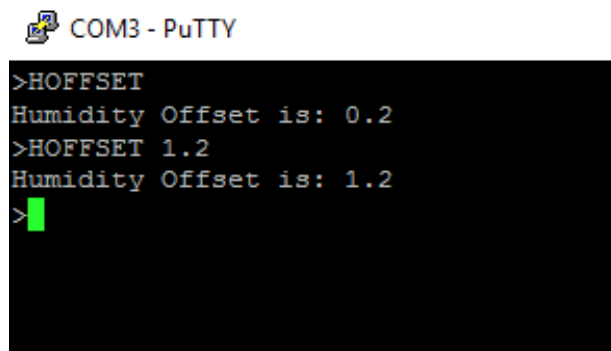

```
COM3 - PuTTY
>HOFFSET
Humidity Offset is: 0.2
>HOFFSET 1.2
Humidity Offset is: 1.2
>
```

# SAFETY WARNING

## GENERAL SAFETY INFORMATION

- Read all provided and available safety information before you use the Model 1000 SP.
- Carefully read all available instructions.
- Use only the power cord and supply approved for the voltage for the Model 1000 SP.
- Replace the power cord if the insulation is damaged or if the insulation shows any signs of wear.
- Make sure the ground conductor in the power cord is connected to a functioning ground.
- Disruption of the ground could put voltage on the chassis that could cause death.
- Use the Model 1000 SP only as specified, or the protection supplied by the Product can be compromised.
- Do not put the Model 1000 SP where access to the power cord isn't possible.
- Immediately cease using and disable the Model 1000 SP if it is damaged.
- Do not use the Model 1000 SP if it operates in an incorrect way.
- Do not operate the Model 1000 SP with unit casing removed. Hazardous voltage exposure is possible.
- Use only specified GEO Calibration replacement parts.
- The Model 1000 SP may only be repaired by approved technicians.
- The Model 1000 SP reservoir must be completely emptied before shipment.
- Do not use the Model 1000 SP around explosive gas, vapor, or in damp or wet environments.

# SAFETY WARNING

## DISPOSAL SAFETY INFORMATION

### European Union—Disposal Information



The symbol above means that according to local laws and regulations your product and/or its desiccant shall be disposed of separately from household waste. When this product reaches its end of life, take it to a collection point designated by local authorities. The separate collection and recycling of your product and/or its desiccant at the time of disposal will help conserve natural resources and ensure that it is recycled in a manner that protects human health and the environment.

## Locations



**GEO Calibration Inc**  
**2190 Smithtown Avenue, Ronkonkoma, NY 11779, USA**  
Tel.: +001 (631) 471 - 6157 • Fax: +001 (631) 471 - 6158  
support@geocalibration.com • www.geocalibration.com

© GEO Calibration Inc. 2020

# REPAIRS

## UNIT REPAIR PROCEDURES

- **Contact GEO Calibration and request an RMA #**
- **Have the Product information ready such as the purchase date and serial number to schedule the repair**
- **Ship the unit to GEO in the original shipping container or one designed specifically for “Safe Travel”**
- **Apply your RMA # on the outside of the shipping package in large numbers**
- **Apply the top right portion of your quotation with RMA # and barcode to the outside of the shipping package, so that it is visible**
- **Include a copy of all GEO communication documentation inside your package**
- **Estimated Return Ship-Date is 15 business days from the date both the unit and a valid method of payment is received**
- **On the Purchase Order, please ensure the “Vendor Name” is GEO Calibration Inc., and the address is 2190 Smithtown Avenue, Ronkonkoma NY 11779**
- **Payment Terms are “Immediate Payment” from Date of Invoice, FOB Origin, the respective Dollar Amounts, and any return shipping instructions are completed. (Please, do not send a copy of your internal “Purchase Requisition” as we need the actual “Purchase Order” with the above items included)**
- **Reference the RMA # on the completed PO and forward a copy via fax (631.471.6158) or email to: [service@geocalibration.com](mailto:service@geocalibration.com)**
- **If credit card is being used for payment and has not been provided as yet, please call +1 (631) 471 - 6157 and provide information; referencing your RMA # when you call**
- **\*\* Exception pricing may apply upon evaluation by the service center. If applicable, this will be presented in a formal re-quote before proceeding\*\***
- **Please note that a “Payment Method” must be on file, reviewed and approved before any service work may begin on your item**
- **If you have any questions do not hesitate to call or email us.**

**Please ship the unit to:**

Attn: Repairs  
GEO Calibration Inc.  
2190 Smithtown Avenue  
Ronkonkoma, NY, 11779, USA

# MAINTENANCE

## SERVICE SCHEDULE

- Maintenance Recommendations:**

GEO Calibration recommends that the unit be annually shipped back to our facility for general maintenance.

Daily	Semi-Annual	As Needed
General Cleaning (Use Proper Cleaning Materials)	Control Probe Calibration	Refill Reservoir with Distilled Water
Ensure the Water Reservoir is Filled		Replace Desiccant Canister
Ensure the Desiccant Ports contain at least one fresh canister.		

## ERROR CODES AND DESCRIPTIONS

Error Code	Description
“No Analog Detected”	Internal Hardware Fault Detected
“Internal Probe Fail”	Internal Hardware Fault Detected
“No HumGen Temp”	Temperature probe failure.
“HumGen Low Limit”	The temperature of the ambient environment is too low for unit operation.
“HumGen High Limit”	The humidity generator has exceeded a high unit. Perform maintenance check of ambient environment and water supply.
“EEPROM Cfg Reset”	The unit configuration settings have been reset to factor default.
“EEPROM Cal Reset”	Factory calibration data reset to default.

For questions, please contact GEO Calibration. You may also visit our website at [www.geocalibration.com](http://www.geocalibration.com) for more assistance.

## DESICCANT CHANGE VISUAL GUIDE

### Overview

The Model 1000 SP ships with a fresh desiccant canister. Each time the Model 1000 SP dries the internal volume of air, the desiccant will become more saturated with water. For optimal performance, the user must periodically replenish or replace the used desiccant. The desiccant type is molecular sieve, which may be regenerated by the user through heating or baking. The desiccant reheating will become less effective after several regenerative sessions.

The user must replace the desiccant as soon as they see drying performance begin to degrade. To aid in this process, the Model 1000 SP has an on-screen indicator that displays once sub par drying performance is detected. In addition to the on-screen indicator, the desiccant itself also contains a chemical that changes color from blue to pink when saturated with water. The user should change the desiccant once approximately 75% of the molecular sieve has changed in color from blue to pink.

### Desiccant Change Procedure

We advise that you purchase extra replacement desiccant canisters directly from GEO Calibration. It is possible to purchase the desiccant in bulk, disassemble the canister and replace the used desiccant with unused desiccant, however, this procedure requires the user to carefully re-assemble the desiccant canister. If this re-assembly is done incorrectly, then air leaks may occur and the unit performance may suffer.

For visual instructions on how to perform a refill of a desiccant canister, please see the next page.

Additional instructions can also be found on the website of the desiccant supplier.

<https://secure.drierite.com/catalog3/page19b.cfm>

## REPLACING THE CANISTER



### 1. Power Off the Unit

Ensure that the unit is powered off before proceeding with a desiccant change.



### 2. Loosen Hook & Loop Straps



### 3. Firmly Grasp Desiccant

This will cause the old desiccant canister to slide from the female adapters. Remove this desiccant completely from the housing and set aside.



### 4. Locate New Desiccant Canister

Remove the used desiccant canister and replace with the fresh desiccant canister.





## 5. Firmly Insert Desiccant Canister

Ensure the hose barbs properly line up with the sockets on the inside of the desiccant housing.



## 6. Press with Force

Firmly press the seal with both thumbs into the canister housing.



## 7. Secure Hook & Loop Straps

## REFILLING DESICCANT CANISTER




### 1. Remove Desiccant

Follow the initial steps from the previous section entitled “Desiccant Change”.



### 2. Open Top Cover of Desiccant

Save the spring, the sieve and the three white felt filters. Discard previous desiccant. Wipe the inside of the desiccant cannister with a clean cloth. Beat filters clean of debris. Clean the sieve and the spring.

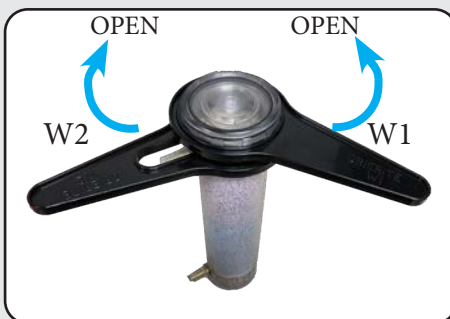

### PLEASE NOTE:

If the cap is too tight, use the desiccant wrenches to loosen the cap.


The method of using wrenches please see the figure on the left.



### 3. Fill Canister with Desiccant

Put the white filter at the bottom. Put the white desiccant inside. Gently tap. Put another filter. Add blue desiccant. Put one more filter. Put one more sieve. Put the spring. Tighten the cover.

## DRAINING THE RESERVOIR

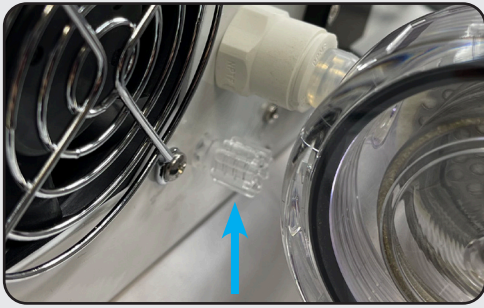

### 1. Locate the Main Drain Port

Turn the cap counter-clockwise to remove.



### 2. Move the Unit to Table Edge

Position a bowl shaped object underneath the unit to catch the drained water.



### 3. Remove the Drain Cap

Tilt the unit to ensure maximum water removal.



### 4. Replace & Tighten Drain Cap


Tighten the drain cap in a clockwise motion. Ensure that the drain cap has a tight seal and no water is leaking.

## CONDENSATION IN THE CHAMBER



### 1. Power Off the Unit

Ensure that the unit is powered off. This is so that no desiccant is wasted while the unit is not in operation.

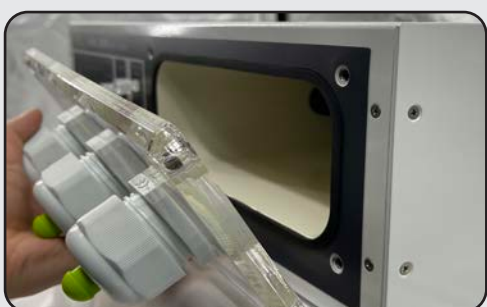

### 2. Open the Chamber Door


Follow the door opening procedure from the quick start guide.



### 3. Remove Condensation

Clean all condensation with an absorbent cloth such as a paper towel or bath towel.

## CHANGING THE CONTROL PROBE

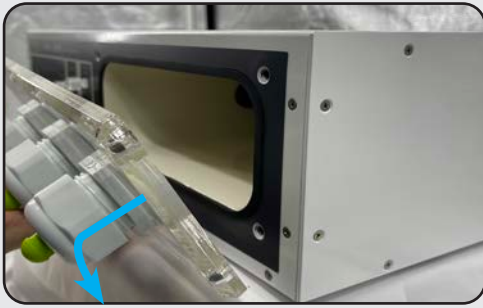

### 1. Open Chamber Door

Turn the screws counter-clockwise to loosen.  
Remove the door.




### 2. Loosen Metal Connector

Twist towards the chamber opening to loosen.



### 3. Remove Probe Head

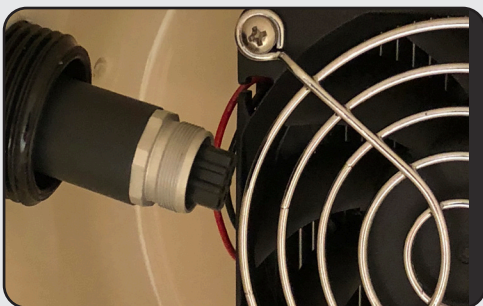

### 4. Locate Probe Connector



## 5. Press Probe into Connector

Slowly rotate the probe head as you press into the cabling body. You will feel the probe “seat” itself once the male - female parts align.



## 6. Secure Metal Connector

Twist the metal connector away from the chamber entrance to secure the probe head to the probe cabling body.

# INDUSTRIES

---

PHARMACEUTICAL  
MANUFACTURING

CALIBRATION LABS

BIOMEDICAL

R&D  
FACILITIES

FOOD PRODUCTION

AUTOMOTIVE  
MANUFACTURING

AEROSPACE

HOSPITAL / MEDICAL

CLEAN ROOMS

For a complete product and accessory review,  
please visit our website: [www.geocalibration.com](http://www.geocalibration.com)



CONTACT US:

---



Email: [Sales@GeoCalibration.com](mailto:Sales@GeoCalibration.com)


Website: [www.GeoCalibration.com](http://www.GeoCalibration.com)



**GEO**  
*Calibration*

**Humidity Control Company**



Proudly Made in the USA 

Email: [Sales@GeoCalibration.com](mailto:Sales@GeoCalibration.com) Website: [www.GeoCalibration.com](http://www.GeoCalibration.com)