


Description	Pulse101A
Maximum Pulse Rate	10KHz
Input Range	0 to 30VDC continuous
Input Low	<0.4 V
Input High	>2.8 V
Internal Weak Pull-Up	<60 μ A
Input Impedance:	>60k Ω
Minimum Pulse Width/ Contact Closure Duration:	\geq 10 microseconds
Reading Rate	1 reading every second up to 1 reading every 24 hours
Memory	500,000 readings 250,000 readings in repeatable start/stop mode
Wrap Around	Yes
LED Indicator	Red & Green
Required Interface Package	IFC200
Baud Rate	115,200
Typical Battery Life	10 years at a 15 minute reading rate
Operating Environment	-40 $^{\circ}$ C to +80 $^{\circ}$ C (-40 $^{\circ}$ F to +176 $^{\circ}$ F), 0 %RH to 95 %RH non-condensing
Material	ABS plastic
Dimensions	1.4 in x 2.5 in x 0.6 in (36 mm x 64 mm x 16 mm)
Weight	0.9 oz (24 g)
Approvals	CE

Battery Warning

WARNING: FIRE, EXPLOSION, AND SEVERE BURN HAZARD. DO NOT SHORT CIRCUIT, CHARGE, FORCE OVER DISCHARGE, DISASSEMBLE, CRUSH, PENETRATE OR INCINERATE. BATTERY MAY LEAK OR EXPLODE IF HEATED ABOVE 80 $^{\circ}$ C (176 $^{\circ}$ F).

Specifications subject to change.

See MadgeTech's terms and conditions at www.madgetech.com

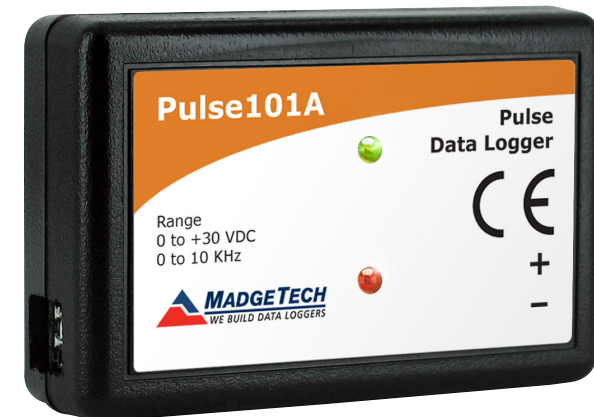

Pulse101A
Pulse Data Logger

MadgeTech, Inc.


6 Warner Road • Warner, NH 03278
Phone 603.456.2011 • Fax 603.456.2012
www.madgetech.com • info@madgetech.com

DOC-1212035-00 REV 6 2014.07.30

Wiring the Data Logger

Wiring Options

The Pulse101A has a two-position removable screw terminal connection. It accepts 2-wire configurations.



Warning: Note the polarity instructions. Do not attach wires to the wrong terminals.

The Pulse101A records the number of pulse inputs or contact closures on the input of the device. The input is continuously sampled at 10 kHz, therefore, the input pulse must be at least 10 microseconds in duration. The counter is reset at the beginning, and the count is recorded at the end of each sample interval.

Note: An input voltage of greater than 30 volts DC on the input could cause loss of data or damage to data logger.

Product Notes

LEDs

- Green LED blinks: 10 seconds to indicate logging, 15 seconds to indicate delay start mode
- Red LED blinks: 10 seconds to indicate low battery and/or memory

Engineering Units

Native measurement units can be scaled to display measurement units of another type. This is useful when monitoring voltage outputs from different types of sensors such as wind speed and flow rate. Please refer to the application note "Engineering Units", found on the MadgeTech website, for information on how to manage Engineering Units. Also view the Engineering Units Video for step-by-step setup instructions.

Password Protection

An optional password may be programmed into the device to restrict access to configuration options. Data may be read out without the password.

Multiple Start/Stop Mode Activation

- To start device: Press and hold the pushbutton for 5 seconds, the green LED will flash during this time. The device has started logging.
- To stop the device: Press and hold the pushbutton for 5 seconds, the red LED will flash during this time. The device has stopped logging.

Installation Guide

Installing the Interface cable

- IFC200: Insert the device into a USB port. The drivers will install automatically.

Installing the software

Insert the Software USB Stick in an open USB port. If the autorun does not appear, locate the drive on the computer and double click on **Autorun.exe**. Follow the instructions provided in the Wizard.

Device Operation

Connecting and Starting the data logger

- Once the software is installed and running, plug the interface cable into the data logger.
- Connect the USB end of the interface cable into an open USB port on the computer.
- The device will appear in the Connected Devices list, highlight the desired data logger.
- For most applications, select "**Custom Start**" from the menu bar and choose the desired start method, reading rate and other parameters appropriate for the data logging application and click "**Start**". (*"Quick Start" applies the most recent custom start options, "Batch Start" is used for managing multiple loggers at once, "Real Time Start" stores the dataset as it records while connected to the logger.*)
- The status of the device will change to "**Running**", "**Waiting to Start**" or "**Waiting to Manual Start**", depending upon your start method.
- Disconnect the data logger from the interface cable and place it in the environment to measure.

Note: The device will stop recording data when the end of memory is reached or the device is stopped. At this point the device cannot be restarted until it has been re-armed by the computer.

Downloading data from a data logger

- Highlight the data logger in the Connected Devices list. Click "**Stop**" on the menu bar.
- Once the data logger is stopped, with the logger highlighted, click "**Download**". You will be prompted to name your report.
- Downloading will offload and save all the recorded data to the PC.

Device Maintenance

Battery Replacement

Materials: Small Phillips Head Screwdriver and Replacement Battery (LTC-7PN)

- Puncture the center of the back label with the screw driver and unscrew the enclosure.
- Remove the battery by pulling it perpendicular to the circuit board.
- Insert the new battery into the terminals and verify it is secure.
- Screw the enclosure back together securely.

Note: Be sure not to over tighten the screws or strip the threads.

Recalibration

The Pulse101A has a digital input signal and cannot be calibrated. A certificate of conformance can be provided.

To send the devices back, visit www.madgetech.com, select Services then RMA Process.